


# PULSELab Pulse measurement software



PULSELab is a software application designed for the measurement of electromagnetic field, current and voltage pulses. PULSELab has been especially developed to help test operators during complex EMP or HPEM immunity tests. PULSELab enables, however, a wider range of applications in the pulse measurement domains.

PULSELab controls the oscilloscope, collects measured data, and processes the data for display and automatic report generation.

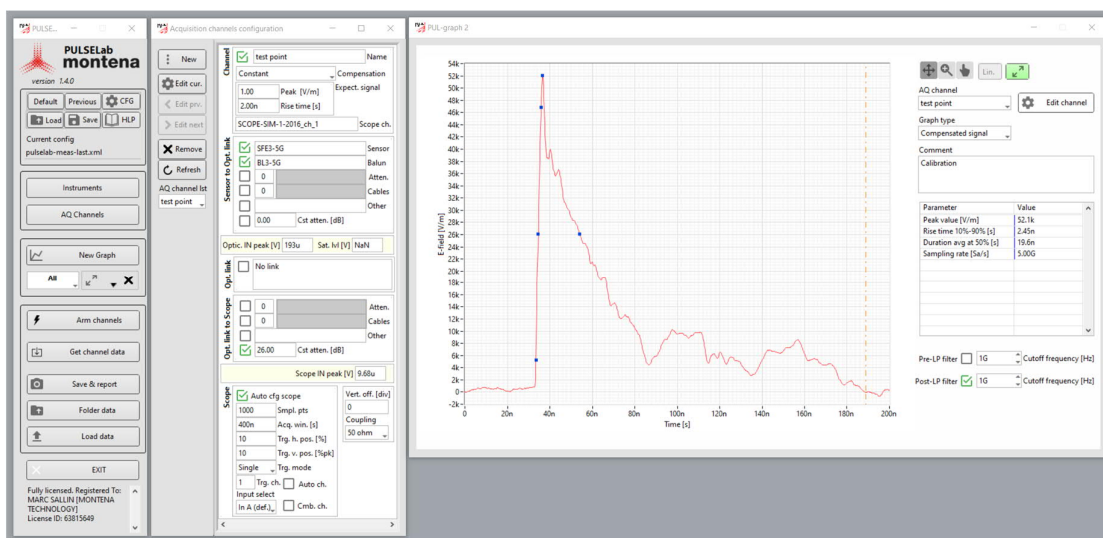

PULSELab improves the measurement accuracy by considering the transfer function of all devices used in the measurement chain (sensor, balun, attenuators, cables, fiber-optic links, etc.) and compensates the signals received by the oscilloscope to display the measured value in its own units. The correction factor of each component can be either a constant value or a frequency dependant transfer function.

The measured pulses are displayed with their main characteristics, such as the peak amplitude, rise-time, fall-time, full-width half-maximum (FWHM) and the peak derivative.

The operator has the possibility to easily generate reports and include test information such as EUT name, test date, operator name, location, comments, etc.

Models and numbers of supported oscilloscopes

PULSELab can control multiple oscilloscopes simultaneously. The software application is compatible with most of the popular recent models of scopes. Contact montena for the latest compatibility list.

Sales Partner:



**ABSOLUTE EMC** Llc.  
Covering sales in North America  
United States, Mexico, & Canada


absolute-emc.com  
Phone:703-774-7505  
info@absolute-emc.com

## Oscilloscope configuration


All needed oscilloscope settings to measure the pulse waveform (vertical and horizontal ranges, trigger levels, number of points, time window, etc.) can be set from the PULSELab application software. Nevertheless, the operator has the possibility to manually set these parameters on the oscilloscope, and PULSELab will read them back from the scope.

## Data correction/compensation

PULSELab combines the transfer function of each element of the measurement chain with the FFT of the oscilloscope raw data.

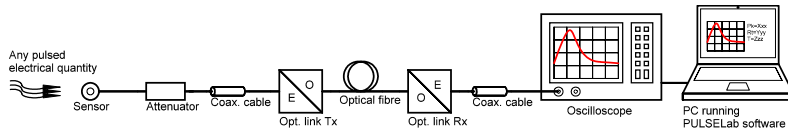

The result is then converted back to the time domain by inverse fast Fourier transform (IFFT). Raw and compensated data can be displayed in both, time and frequency domains, and exported to a text file.

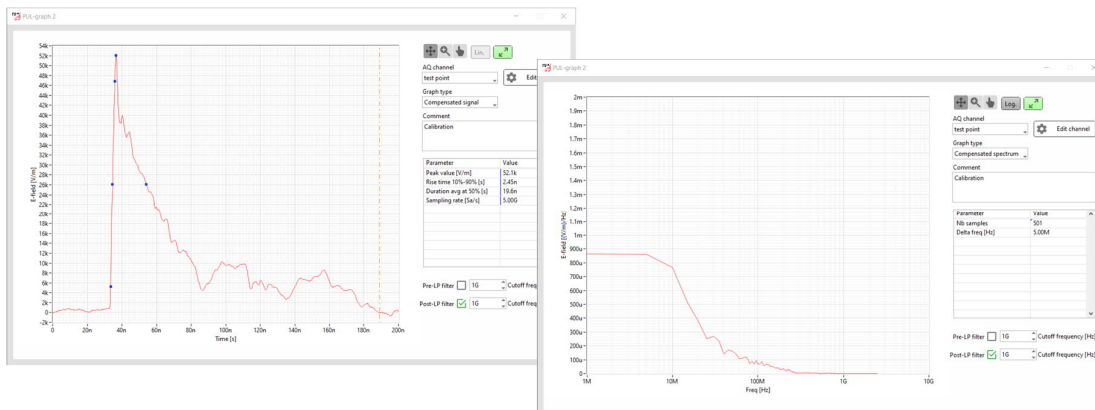

The transfer functions of all montena pulse measurement devices (sensors, baluns, fiber-optic links, ...etc) are preconfigured. The user can create and edit additional components. A more straightforward compensation approach (using constant factor and time-domain integration) can be used too.

## Time delay compensation

When measuring fast pulses at different locations, with different cable or fibre optic lengths, the measurement will be time-shifted because of the pulse propagation time and of the delays induced by cables, fibre optics and electronics. The operator has the possibility to synchronise the display of each channel, based on the pulse peak or other pulse parameters.

## Interface to MOL500T / MOL2000T

Montena MOL500T and MOL2000T are broadband fiber-optic link systems with variable remote-controlled transmission gain. PULSELab interfaces with the fiber-optic link(s), read and set the transmission

Sales Partner:



**ABSOLUTE EMC** Lic.  
Covering sales in North America  
United States, Mexico, & Canada

absolute-emc.com  
Phone:703-774-7505  
info@absolute-emc.com

gain(s) to avoid saturations and ensure the best usage of the dynamic range of the measurement devices.

Save and recall measurement setup's

The configuration and setup of the measurement channels, including the fiber-optic links (MOL) and the oscilloscopes configurations can be saved as setup files and reloaded.



SPECIFICATIONS																											
Type	PULSELab software application																										
Computer hardware requirements	1 x USB port and 1x LAN port Screen resolution of at least 1920 x 1080																										
Computer software requirements	PC with Microsoft Windows 10 or 11																										
Number of channels	There is no limitation of the number of measurement channels and of the number of connected oscilloscopes. Only the communication speed and data processing time may somehow limit the scalability.																										
Supported sensors	Current pulses with current probes / current transformers Current pulses with Rogowski coils Voltage pulses with voltage probes Voltage fast pulses with V-Dot sensors Electromagnetic field pulses with B-Dot and D-Dot sensors Etc.																										
Preconfigured devices responses	Montena B-dot free-space and ground plane field sensors Montena D-dot free-space and ground plane field sensors Prodyn B-24, B-90 field sensors Montena baluns (used with free space field sensors) Montena V-dot high voltage dividers Magnetlab current transformers Pearson current monitor 3025 Montena MOL fibre optic transmission links Montena ITR passive integrators Montena semi-rigid coaxial cable assemblies Other devices and transfer functions can be added by the user.																										
Available pulse measurement parameters	<table border="0"> <tr> <td>[Time domain]</td> <td>[Frequency domain]</td> </tr> <tr> <td>Peak value</td> <td>Max</td> </tr> <tr> <td>Rise time x% - y%</td> <td>Number of samples</td> </tr> <tr> <td>Duration at z%</td> <td>Delta freq</td> </tr> <tr> <td>Max pulse derivative</td> <td>Freq @ max</td> </tr> <tr> <td>Peak on graph</td> <td>Etc.</td> </tr> <tr> <td>Peak rate of rise</td> <td></td> </tr> <tr> <td>Root action</td> <td></td> </tr> <tr> <td>Rectified total impulse</td> <td></td> </tr> <tr> <td>Time @ peak</td> <td></td> </tr> <tr> <td>Sampling rate</td> <td></td> </tr> <tr> <td>Number of samples</td> <td></td> </tr> <tr> <td>Delta t</td> <td></td> </tr> </table>	[Time domain]	[Frequency domain]	Peak value	Max	Rise time x% - y%	Number of samples	Duration at z%	Delta freq	Max pulse derivative	Freq @ max	Peak on graph	Etc.	Peak rate of rise		Root action		Rectified total impulse		Time @ peak		Sampling rate		Number of samples		Delta t	
[Time domain]	[Frequency domain]																										
Peak value	Max																										
Rise time x% - y%	Number of samples																										
Duration at z%	Delta freq																										
Max pulse derivative	Freq @ max																										
Peak on graph	Etc.																										
Peak rate of rise																											
Root action																											
Rectified total impulse																											
Time @ peak																											
Sampling rate																											
Number of samples																											
Delta t																											
Compatible oscilloscopes	Teledyne Lecroy Wave Series Tektronix MDO MSO DPO 2000 3000 4000 Series, MSO5X Series, 7000 Series Rohde & Schwarz RTO1000 RTO2000 RTO6 RTE1000 RTM3000 MXO4 Series Keysight 2000 3000 4000 X-Series, 90000 Series If an oscilloscope series is not listed, please contact montena.																										

montena technology sa 1728 Rossens Switzerland www.montena.com

## Licences and ordering information

PULSELab licences are lifetime fixed licences. One licence per computer is required. The licence activation is semi-automatic during the software installation.

TYPE	DESCRIPTION
PULSELab	Pulse measurement and processing software application, Lifetime license for installation on one PC.

Sales Partner:



**ABSOLUTE EMC** Llc.  
Covering sales in North America  
United States, Mexico, & Canada

absolute-emc.com  
Phone:703-774-7505  
info@absolute-emc.com